

VITA LUMIN[®] VACUUM

VITA Teeth



VITA shade determination

VITA shade communication

VITA shade reproduction

VITA shade control

Date of issue: 08.18

VITA – perfect match.

VITA

Formenkarte · Keramikzähne


Mould Chart · Ceramic denture teeth

Carte de formes · Dents en céramique


Carta de formas · Dientes de cerámica

Tabella delle forme · Denti di ceramica

VITA LUMIN® VACUUM Upper anteriors



schaufelförmig
 ovoid
 en forme de pelle
 en forma di pala
 a forma di pala







dreieckig
 tapering
 triangulaire
 triangular
 triangolare






Lower anteriors




rechteckig
 rectangular
 rectangulaire
 rectangular
 rettangolare

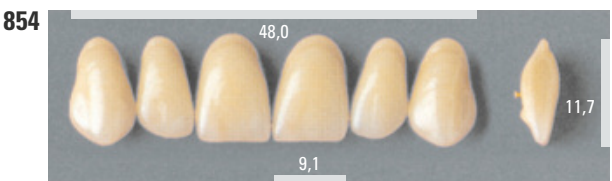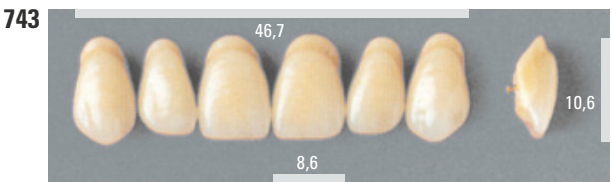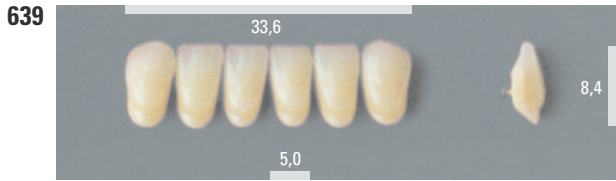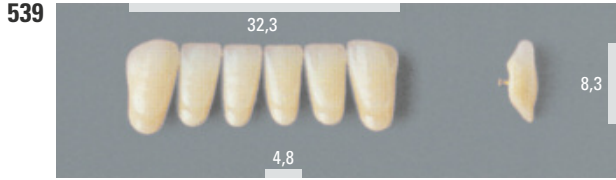

quadratisch
 square
 carré
 cuadrado
 quadrato

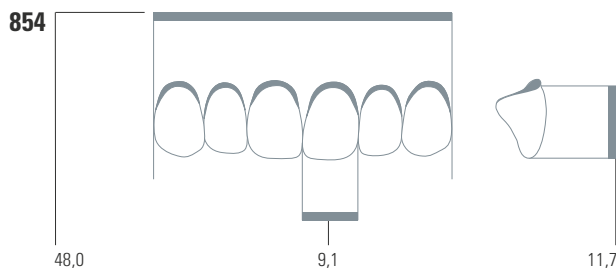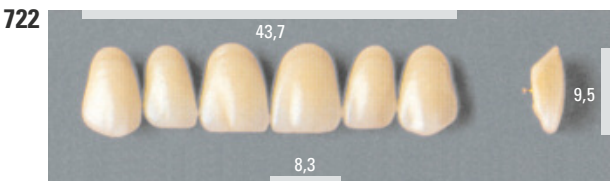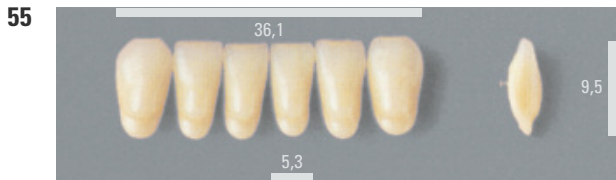

Upper and lower posteriors



CUSPIFORM






SYNOFORM



VITA LUMIN® VACUUM Combination Chart

LUMIN® VACUUM Kombinationstabelle
 LUMIN® VACUUM Combination Chart
 Tableau de Combinaison LUMIN® VACUUM
 Tabla de Combinación LUMIN® VACUUM
 Tabella di Combinazione LUMIN® VACUUM

No.	 mm	No.	 mm	mm	
				No.	 mm
180	44.7 50.7	639	33.6	41C 29.5 31.8	11S 29.3 31.2
182	43.0 48.6	539	32.3	40C 28.3 29.5	10S 28.2 29.7
185	46.1 52.2	730	35.6	44C 32.3 34.3	13S 30.3 32.7
187	44.6 50.2	760	33.6	41C 29.5 31.8	11S 29.3 31.2
190	42.6 48.1	539	32.3	40C 28.3 29.5	10S 28.2 29.7
513	40.1 45.8	539	32.3	40C 28.3 29.5	10S 28.2 29.7
565	45.3 51.4	730	35.6	44C 32.3 34.3	13S 30.3 32.7
612	43.9 49.9	539	32.3	41C 29.5 31.8	11S 29.3 31.2
622	44.1 50.1	639	33.6	41C 29.5 31.8	11S 29.3 31.2
627	42.3 47.8	760	33.6	40C 28.3 29.5	10S 28.2 29.7
632	42.5 48.3	730	35.6	41C 29.5 31.8	11S 29.3 31.2
722	43.7 49.8	639	33.6	41C 29.5 31.8	11S 29.3 31.2
732	44.8 50.5	760	33.6	41C 29.5 31.8	11S 29.3 31.2
734	43.3 49.4	760	33.6	41C 29.5 31.8	11S 29.3 31.2
737	45.7 51.6	730	35.6	44C 32.3 34.3	13S 30.3 32.7
742	46.2 52.2	740	35.1	44C 32.3 34.3	13S 30.3 32.7
743	46.7 52.9	740	35.1	44C 32.3 34.3	13S 30.3 32.7
773	47.1 53.2	639	33.6	44C 32.3 34.3	13S 30.3 32.7
843	47.6 53.6	639	33.6	44C 32.3 34.3	13S 30.3 32.7
854	48.0 54.6	55	36.1	44C 32.3 34.3	13S 30.3 32.7

VITA LUMIN VACUUM Anteriores und Posteriores sind in den VITA classical Farben A1, A2, A3, A3.5, B2, B3, C1, C2, D2, D3 erhältlich.

Für weitere Farben fallen Lieferzeiten an.

VITA LUMIN VACUUM Anteriores and Posteriores are available in the VITA classical shades A1, A2, A3, A3.5, B2, B3, C1, C2, D2, D3.

Further colours are subject to delivery times.

VITA LUMIN VACUUM Anteriores et Posteriores sont disponibles dans les teintes VITA classical A1, A2, A3, A3.5, B2, B3, C1, C2, D2, D3.

Pour toutes les couleurs supplémentaires s'applique un délai de livraison.


I denti VITA LUMIN VACUUM Anteriores e Posteriores sono disponibili in colorazione VITA classical A1, A2, A3, A3.5, B2, B3, C1, C2, D2, D3.

Colori supplementari hanno un tempo di consegna.

La gama VITA LUMIN VACUUM Anteriores y Posteriores está disponible en los colores VITA classical A1, A2, A3, A3.5, B2, B3, C1, C2, D2, D3.

Otros colores tendrán plazo de entrega.

With the unique VITA SYSTEM 3D-MASTER, all natural tooth shades can be systematically determined and perfectly reproduced.

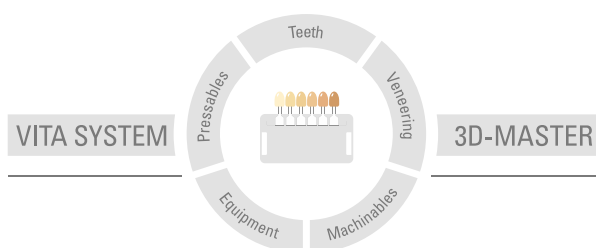

Please note: Our products must be used in accordance with the instructions for use. We accept no liability for any damage resulting from incorrect handling or usage. The user is furthermore obliged to check the product before use with regard to its suitability for the intended area of applications. We cannot accept any liability if the product is used in conjunction with materials and equipment from other manufacturers that are not compatible or not authorized for use with our product and this results in damage. The VITA Modulbox is not necessarily a component of the product. Date of issue of this information: 08.18

After the publication of this information for use any previous versions become obsolete. The current version can be found at www.vita-zahnfabrik.com

VITA Zahnfabrik has been certified in accordance to the Medical Device Directive and the following products bear the CE mark **CE** 0124 :

VITA LUMIN VACUUM Teeth fulfil the requirements of ISO 4824 : 1993.

VITA

VITA Zahnfabrik H. Rauter GmbH & Co.KG
Spitalgasse 3 · D-79713 Bad Säckingen · Germany
Tel. +49(0)7761-562-0 · Fax +49(0)7761-562-299
Hotline: Tel. +49(0)7761-562-222 · Fax +49(0)7761-562-446
www.vita-zahnfabrik.com · info@vita-zahnfabrik.com
[facebook.com/vita.zahnfabrik](https://www.facebook.com/vita.zahnfabrik)